

Kind of Equipment	Optical Power Meter
Type / Model No.	MP-80
Cat Number	ZP-FIT-9014
Serial Number	C2410-7390-053
Manufacturer	JDSU Fiber Inspection & Test
Calibration Date	March 24 , 2010
Confirmation Interval	36 Months
Ambient Temperature / relative humidity	(23±3)°C / (40 ... 60) %

This calibration certificate confirms that all measurements lie within the limit values stated in the product-specific calibration procedure.


This calibration results are traceable to National Standards which are consistent with the recommendations of the General Conference on Weights and Measures (CGPM), or to standards derived from natural constants, or to standards relying on ratio measurements with self-calibrating technique for their calibration. If a National Standard is not available, the result is traceable to the Reference Standard of JDSU.

The metrological confirmation system of measuring equipment complies with ISO 10012-1.

The stated confirmation interval shall be regarded as a recommendation. The real definition of the confirmation interval should be made by the user. The type of application and the environmental conditions should be taken into account.

Date **March 24 , 2010**

Tester 

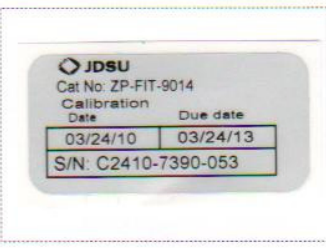

JDSU Fiber Inspection & Test
18421 Bothell-Everett Hwy, Suite 110
Mill Creek, WA 98012
(425) 398-1298